

FIG. 3

300

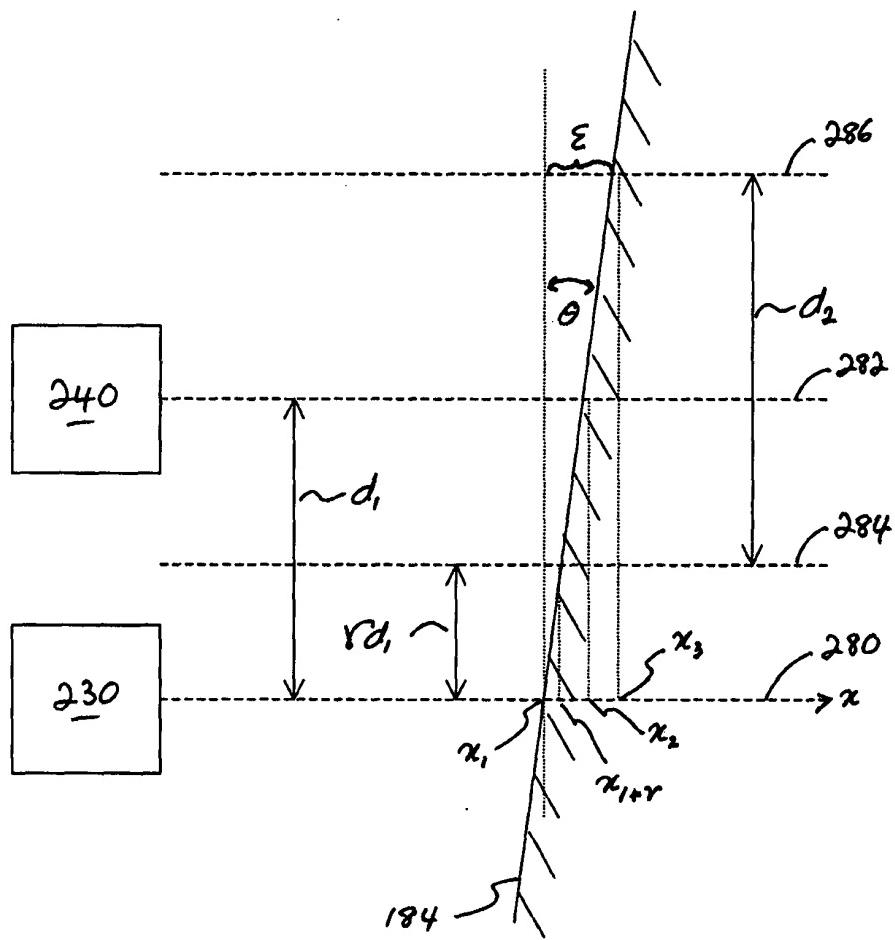


FIG. 4

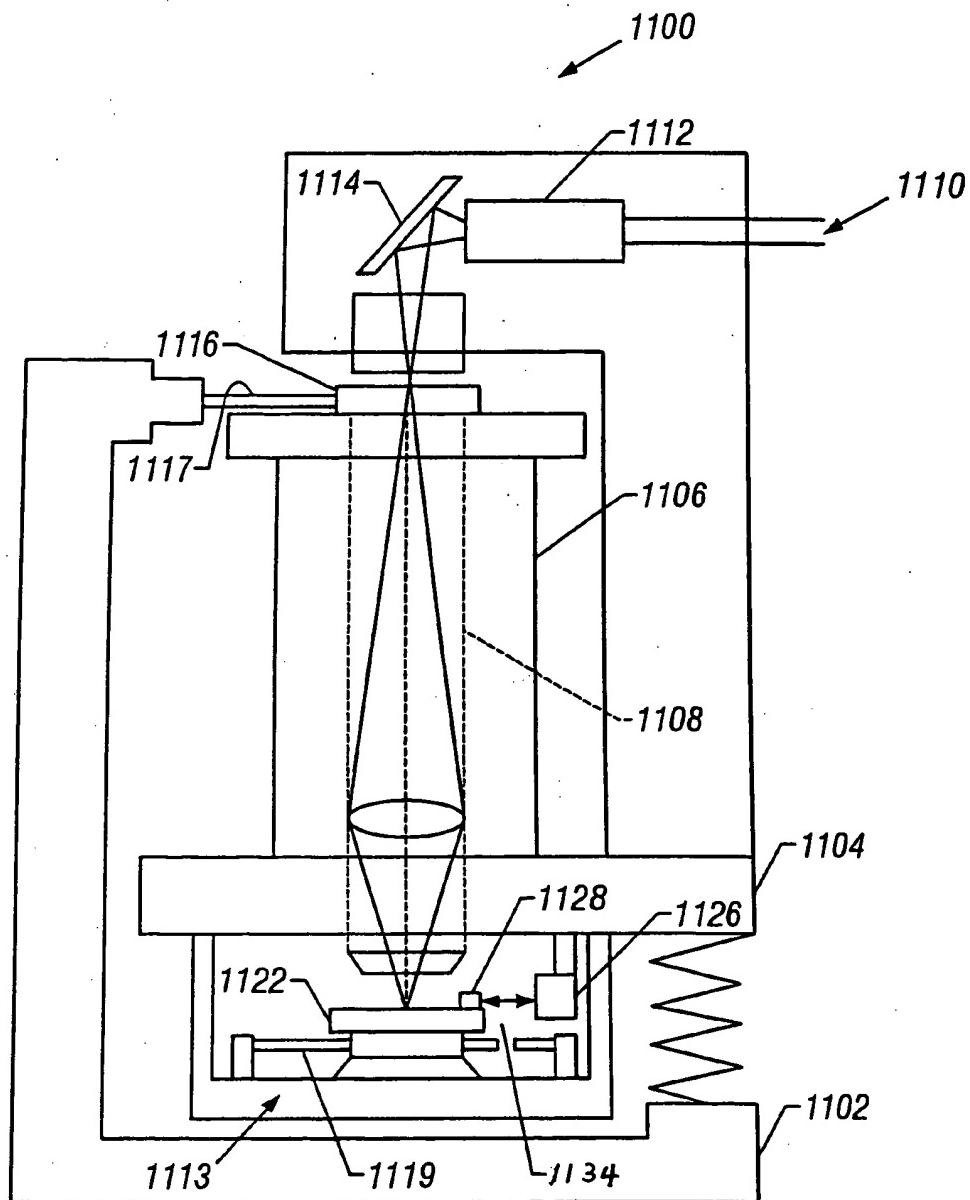


FIG. 5

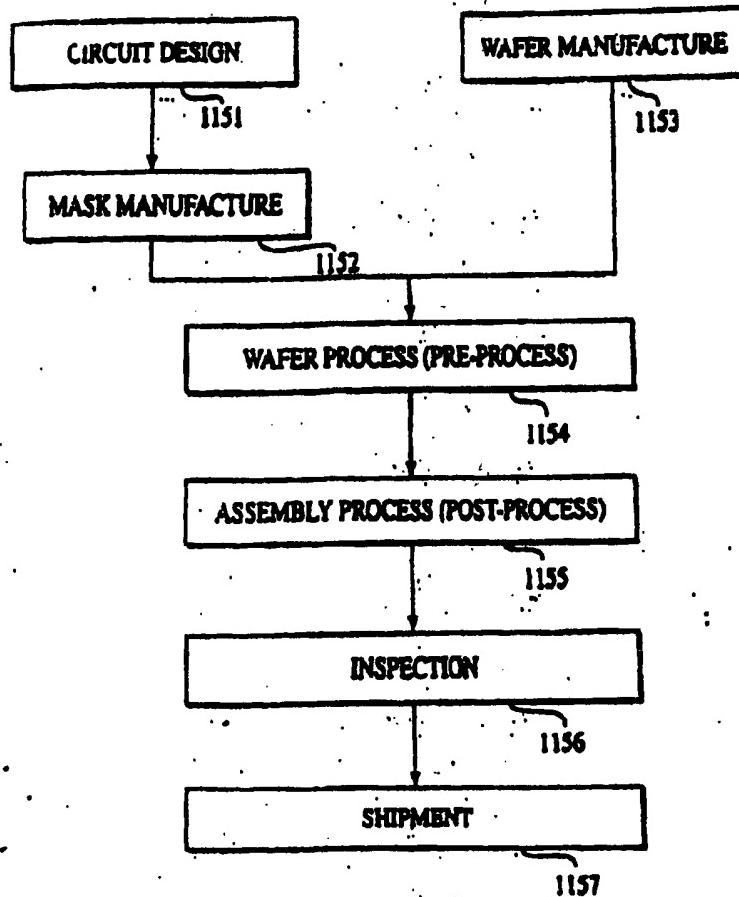


FIG. 6(a)

Applicant(s): Henry A. Hill

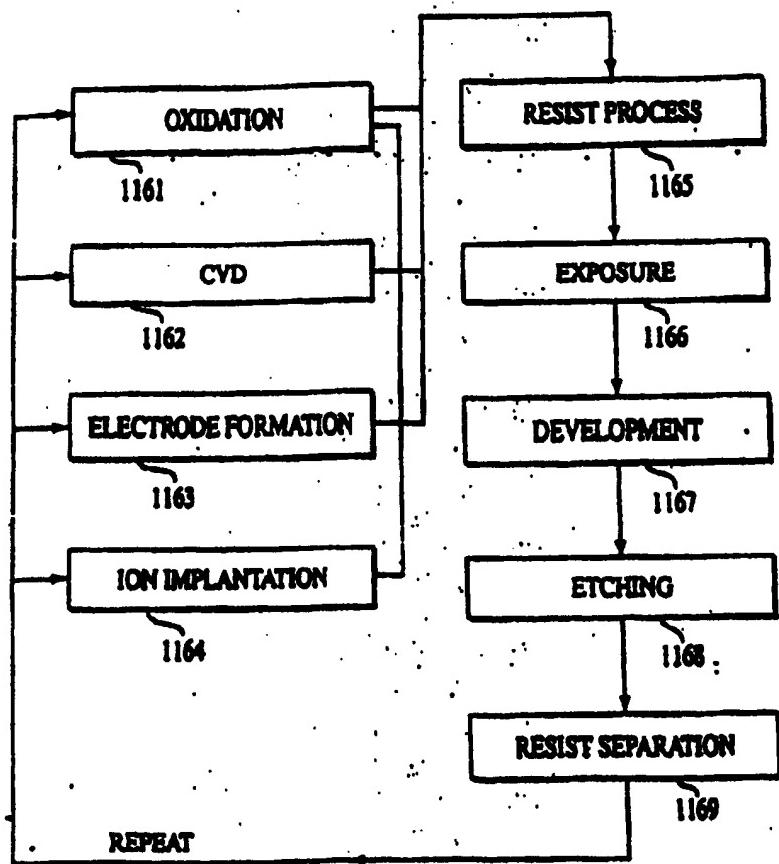
MEASUREMENT AND COMPENSATION OF ERRORS IN
INTERFEROMETERS

FIG. 6(6)

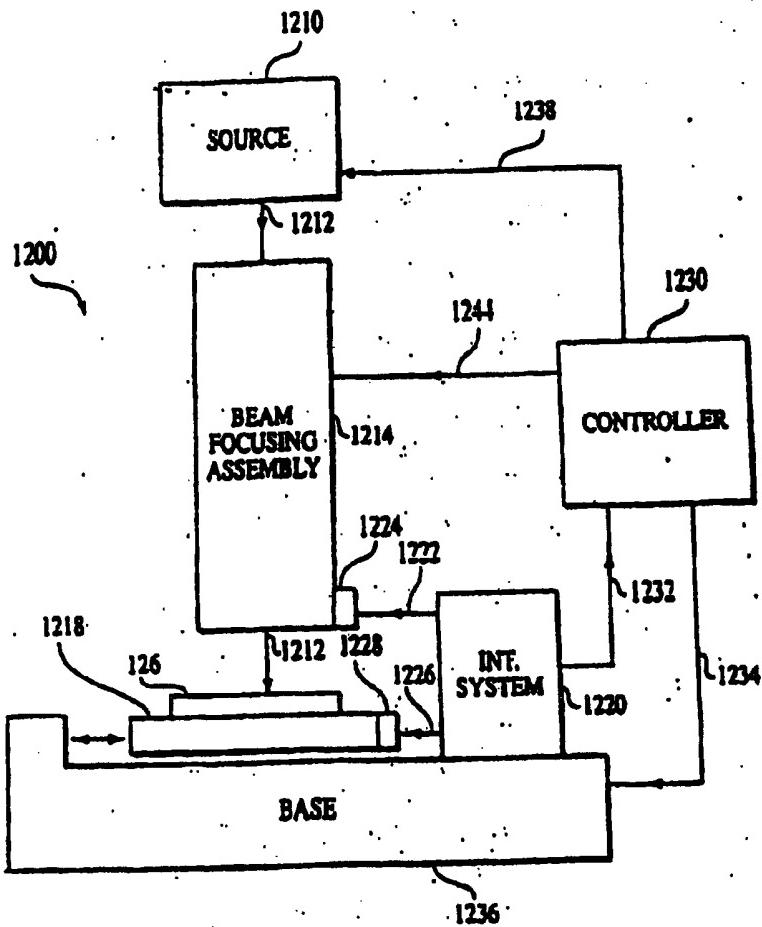


FIG. 7